


See and Treat Hysteroscopy
without capital cost
or complexity



LiNA OperåScope™


Single-Use Operative Hysteroscopy System

The complete system for see and treat
hysteroscopy in the office setting.



The value of “see and treat” hysteroscopy to both patients and providers has been well established for decades.¹

However, it’s estimated that less than 20% of gynecologists currently perform hysteroscopy in the office.²

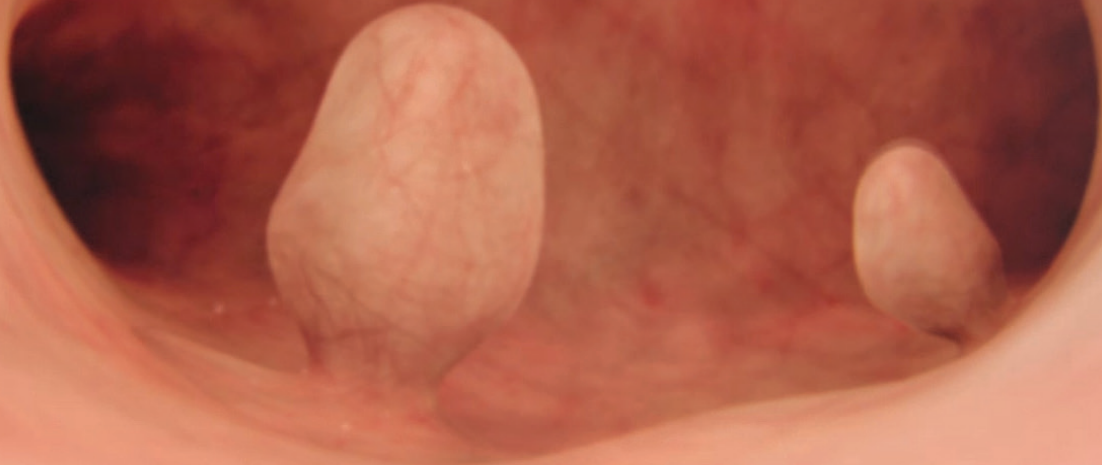

Traditional hysteroscopy can be complicated...

The cost and complexity of traditional equipment can make it difficult to incorporate hysteroscopy into your practice. You need staff, sterilization chemicals, and supplies... lots of supplies if you want to support multiple rooms and multiple patients in a day.^{3,4}




Turn every exam room
into a hysteroscopy
procedure room.



LiNA OperaScope™

The LiNA OperaScope™ was designed specifically with the office setting in mind. The convenient single-use design is ready for use out of the box, allowing you to diagnose and treat patients without the constraints of traditional hysteroscopy.⁴

Curved tip to match her anatomy.
Ergonomic handle to match yours.

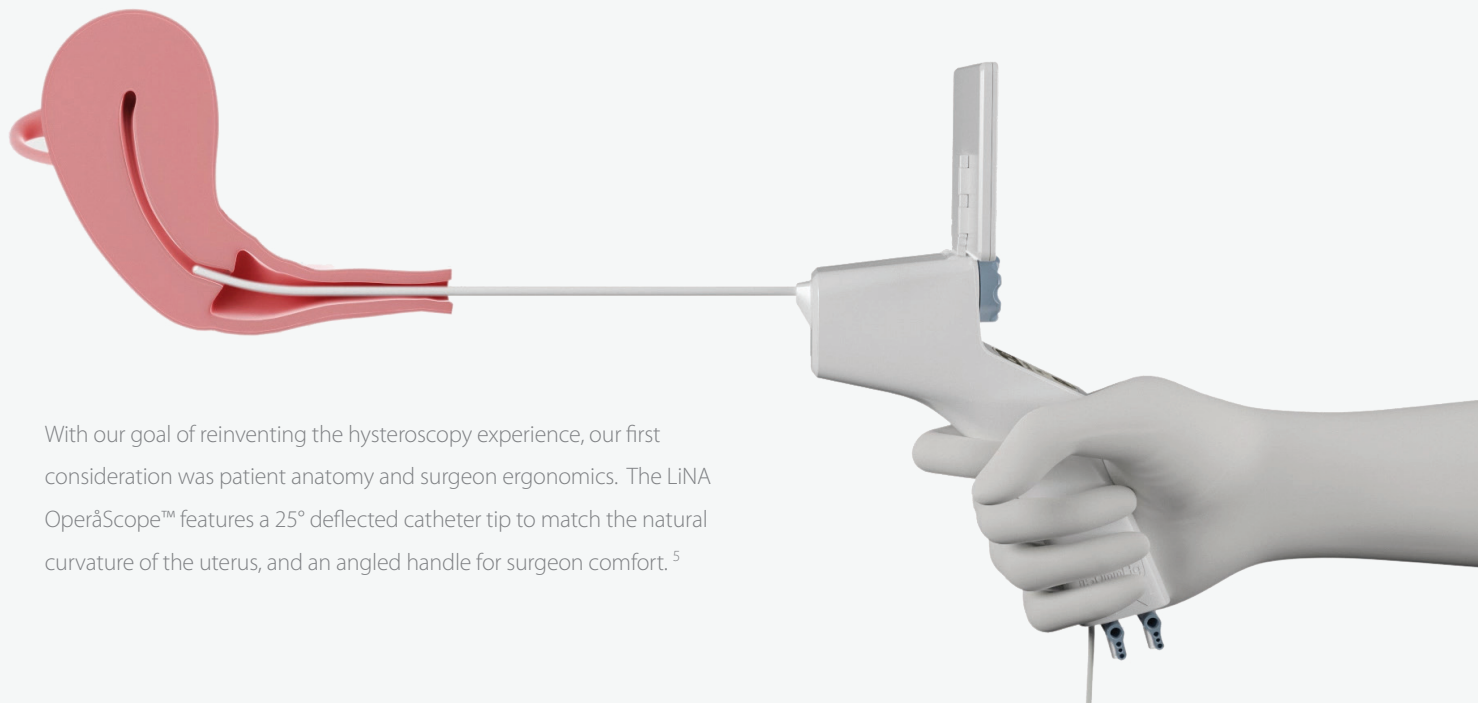


With our goal of reinventing the hysteroscopy experience, our first consideration was patient anatomy and surgeon ergonomics. The LiNA OperāScope™ features a 25° deflected catheter tip to match the natural curvature of the uterus, and an angled handle for surgeon comfort.⁵

The steerability and control
you've been looking for.

Our rigid catheter and 360° steerable tip allows for
precise control and maneuverability to navigate your
patient's unique anatomy.



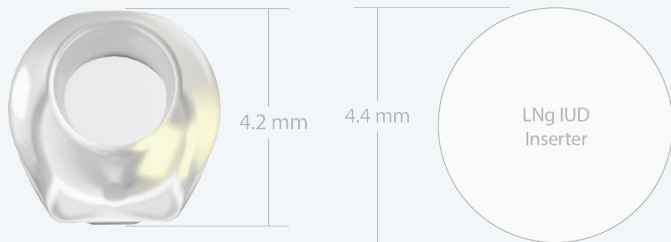

Slim catheter for less dilation and anesthesia.

State of the art micro camera technology has allowed us to create a catheter tip that's smaller than a LNg IUD inserter for improved patient tolerability.^{6,7}



Max
150mmHg

Effective distention and
clear visualization.

LiNA OperåScope™ features dedicated in-flow
and out-flow channels with individual stop-
cocks for optimal fluid management.



LiNA Tubing and Drape Kit.


We offer a convenient hysteroscopy tubing and drape kit to address your fluid management needs. Our kit includes:

Full underbuttock drape with graduation markings and drainage port.

Inflow tubing with luer lock connector and spike connector for use with saline bag.

Outflow tubing with luer lock connector and female suction cannister connector.

Drainage collection bag.

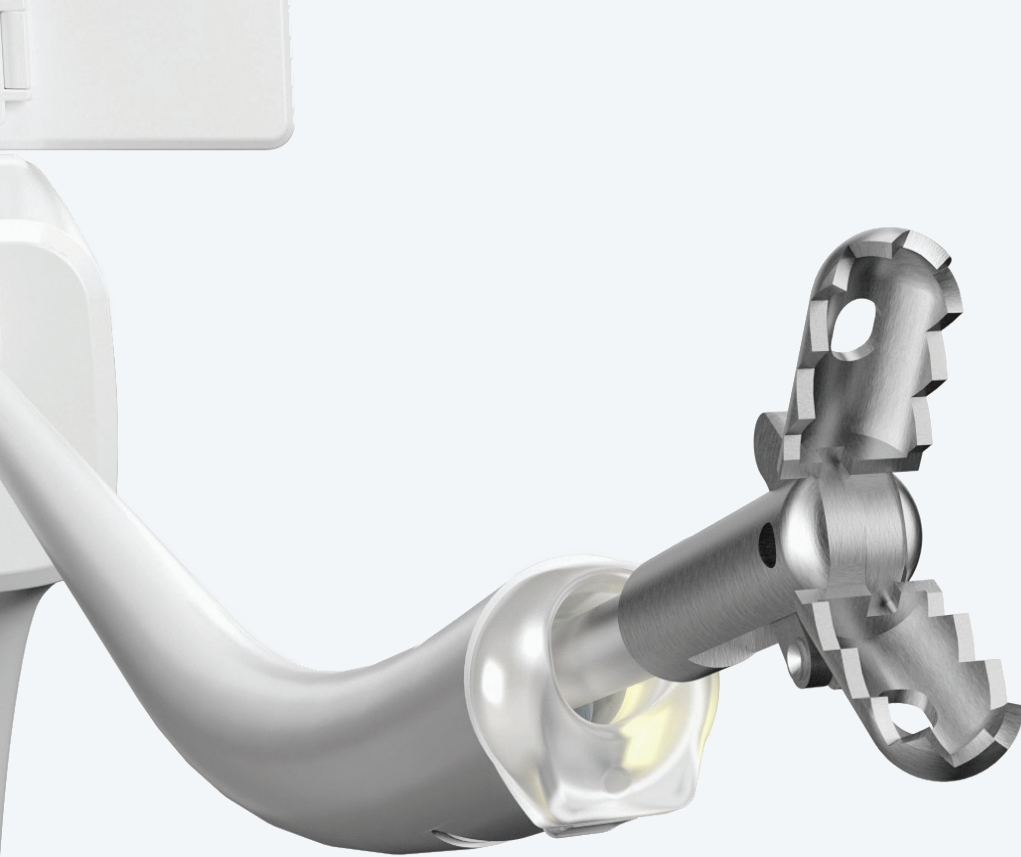

LiNA Single-Use Instrumentation.

LiNA OperâScope™ features a 5.5 french operative channel for therapeutic use. Our affordable selection of single-use instrumentation enables see and treat hysteroscopy without the constraints of traditional reusable instruments.⁴

Biopsy Cup Forceps
Rat Tooth Alligator Grasper
Scissors



Recording and Connectivity.

The LiNA OperåScope™ offers multiple options to meet your office setup and recording needs. You have the flexibility of onboard LCD viewing only, connection directly to an external monitor via standard HDMI cable, or utilize the LiNA OperåScope™ Recording Module for image and video capture to USB.



Product Code	Description	UOM
OP-201-6	LiNA OperâScope™ Operative Hysteroscope with HDMI cable and onboard LCD (sterile single-use)	Box of 6ea
OP-FCP-6	LiNA OperâScope™ Biopsy Cup Forceps (sterile single-use)	Box of 6ea
OP-GRA-6	LiNA OperâScope™ Rat Tooth Alligator Grasper (sterile single-use)	Box of 6ea
OP-SCI-6	LiNA OperâScope™ Scissors (sterile single-use)	Box of 6ea
OP-TDK-6	LiNA OperâScope™ Tubing and Drape Kit (sterile single-use)	Box of 6ea
OP-RM-1	LiNA OperâScope™ Recording Module	Each

References:

1. Bettocchi, S. Instrumentation in Office Hysteroscopy. In: LD Bradley and T Falcone, eds. Hysteroscopy. Office evaluation and management of the uterine cavity. Philadelphia: Mosby Elsevier; 2009: 3
2. Salazar, Christina Alicia et al. Office Operative Hysteroscopy: An Update. Journal of Minimally Invasive Gynecology, Volume 25, Issue 2, 199 - 208
3. Franchini, Mario et al. Hysteroscopic Endometrial Polypectomy: Clinical and Economic Data in Decision Making. Journal of Minimally Invasive Gynecology, Volume 25, Issue 3, 418 - 425
4. General Reprocessing Instructions for KARL STORZ Products (USA) PI-000035-20.1 2-03-11
5. Sallam HN, Agameya AF, Rahman AF, et al. Ultrasound measurement of the uterocervical angle before embryo transfer: A prospective controlled study. Hum Reprod. 2002;17(7):1767–1772.
6. Overcoming barriers to levonorgestrel-releasing intrauterine system placement: an evaluation of placement of LNG-IUS 8 using the modified Evolver®. Contraception, 96(6), 426-431.
7. Bednarek, P. H., & Jensen, J. T. (2009). Safety, efficacy and patient acceptability of the contraceptive and non-contraceptive uses of the LNG-IUS. International Journal of Women's Health, 1, 45–58

Innovation in Gynecology

LiNA Medical Formervangen 5, DK-2600 Glostrup, Denmark

Tel: 1 (855) 546-2633 | info@linamed.com | www.linamed.com

©2018 LiNA Medical International Operations. All rights reserved. All products may not be available for sale in all geographies. Please contact your local LiNA Medical representative for information about products available in your area. This information is intended for healthcare professionals. If you are a patient seeking more information, please consult your healthcare provider. Before using any LiNA product, always refer to the IFU included in our packaging for complete indications for use, contraindications, warnings, precautions, and instructions.

LiNA OperaScope Physician Brochure 4/2018

